

Anti-CD31 antibody [JC/70A] ab9498

★★★★★ **39 Abreviews** **210 References** 画像数 10

製品の概要

製品名	Anti-CD31 antibody [JC/70A]
製品の詳細	Mouse monoclonal [JC/70A] to CD31
由来種	Mouse
アプリケーション	適用あり: IHC-Fr, WB, IHC-P, Flow Cyt, ICC/IF
種交差性	交差種: Human 交差が予測される動物種: Cynomolgus monkey 
免疫原	Tissue, cells or virus. This information is proprietary to Abcam and/or its suppliers.
ポジティブ・コントロール	WB: HUVEC and HeLa whole cell lysate. Human spleen and kidney tissue lysate. IHC-P: Human tonsil tissue. ICC/IF: HUVEC cells. Flow Cyt: PBMC.
特記事項	<p>This antibody clone is manufactured by Abcam. If you require a custom buffer formulation or conjugation for your experiments, please contact orders@abcam.com.</p> <p>The Life Science industry has been in the grips of a reproducibility crisis for a number of years. Abcam is leading the way in addressing this with our range of recombinant monoclonal antibodies and knockout edited cell lines for gold-standard validation. Please check that this product meets your needs before purchasing.</p> <p>If you have any questions, special requirements or concerns, please send us an inquiry and/or contact our Support team ahead of purchase. Recommended alternatives for this product can be found below, along with publications, customer reviews and Q&As</p>

製品の特性

製品の状態	Liquid
保存方法	Shipped at 4°C. Store at +4°C short term (1-2 weeks). Upon delivery aliquot. Store at -20°C long term. Avoid freeze / thaw cycle.
バッファー	Preservative: 0.02% Sodium azide Constituents: PBS, 6.97% L-Arginine
精製度	Protein G purified
ポリ/モノ	モノクローナル
クローン名	JC/70A
ミエローマ	unknown

アイソタイプ IgG1
軽鎖の種類 kappa

アプリケーション

The Abpromise guarantee Abpromise保証は、次のテスト済みアプリケーションにおけるab9498の使用に適用されます
アプリケーションノートには、推奨の開始希釈率がありますが、適切な希釈率につきましてはご確認ください。

アプリケーション	Abreviews	特記事項
IHC-Fr	★★★★★ (3)	Use a concentration of 1 µg/ml.
WB	★★★★★ (1)	1/1000. Detects a band of approximately 130 kDa (predicted molecular weight: 82 kDa). Treat samples with PNGase F or phosphatase to confirm the specificity of bands if necessary. The observed band size of CD31 may not be the same as predicted MWs in WB due to the different forms and modifications of CD31.
IHC-P	★★★★★ (26)	Use a concentration of 0.5 µg/ml. Perform heat mediated antigen retrieval with citrate buffer pH 6 before commencing with IHC staining protocol. The ideal fixation time will depend on the size of the tissue block and the type of tissue, but fixation between 18–24h is suitable for most samples. Positive Control: Human tonsil tissue
Flow Cyt	★★★★★ (1)	1/20.
ICC/IF	★★★★★ (2)	Use a concentration of 1 µg/ml. It is recommended to incubate cells with 0.1% Triton-X for 5 min to detect nuclear antigen. Use 0.3M glycine to quench autofluorescence caused by aldehydes. Positive Control: HUVEC cells

ターゲット情報

機能 Induces susceptibility to atherosclerosis (By similarity). Cell adhesion molecule which is required for leukocyte transendothelial migration (TEM) under most inflammatory conditions. Tyr-690 plays a critical role in TEM and is required for efficient trafficking of PECAM1 to and from the lateral border recycling compartment (LBRC) and is also essential for the LBRC membrane to be targeted around migrating leukocytes. Prevents phagocyte ingestion of closely apposed viable cells by transmitting 'detachment' signals, and changes function on apoptosis, promoting tethering of dying cells to phagocytes (the encounter of a viable cell with a phagocyte via the homophilic interaction of PECAM1 on both cell surfaces leads to the viable cell's active repulsion from the phagocyte. During apoptosis, the inside-out signaling of PECAM1 is somehow disabled so that the apoptotic cell does not actively reject the phagocyte anymore. The lack of this repulsion signal together with the interaction of the eat-me signals and their respective receptors causes the attachment of the apoptotic cell to the phagocyte, thus triggering the process of engulfment).

Isoform Delta15 is unable to protect against apoptosis. Modulates BDKRB2 activation. Regulates bradykinin- and hyperosmotic shock-induced ERK1/2 activation in human umbilical cord vein cells (HUVEC).

組織特異性

Expressed on platelets and leukocytes and is primarily concentrated at the borders between endothelial cells. Isoform Long predominates in all tissues examined. Isoform Delta12 is detected only in trachea. Isoform Delta14-15 is only detected in lung. Isoform Delta14 is detected in all tissues examined with the strongest expression in heart. Isoform Delta15 is expressed in brain, testis, ovary, cell surface of platelets, human umbilical vein endothelial cells (HUVECs), Jurkat T-cell leukemia, human erythroleukemia (HEL) and U937 histiocytic lymphoma cell lines (at protein level).

配列類似性

Contains 6 Ig-like C2-type (immunoglobulin-like) domains.

ドメイン

The Ig-like C2-type domains 2 and 3 contribute to formation of the complex with BDKRB2 and in regulation of its activity.


翻訳後修飾

Phosphorylated on Ser and Tyr residues after cellular activation. In endothelial cells Fyn mediates mechanical-force (stretch or pull) induced tyrosine phosphorylation.

細胞内局在

Membrane. Cell junction. Localizes to the lateral border recycling compartment (LBRC) and recycles from the LBRC to the junction in resting endothelial cells and Cell junction. Localizes to the lateral border recycling compartment (LBRC) and recycles from the LBRC to the junction in resting endothelial cells.

画像

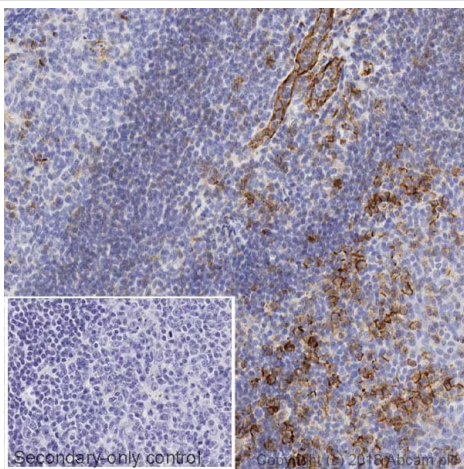


Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-CD31 antibody [JC/70A] (ab9498)

IHC image of CD31 staining in a section of formalin-fixed paraffin-embedded normal human tonsil* performed on a Leica BOND™ system using the standard protocol F. The section was pre-treated using heat mediated antigen retrieval with sodium citrate buffer (pH6, epitope retrieval solution 1) for 20mins. The section was then incubated with ab9498, 0.5ug/ml, for 15 mins at room temperature and detected using an HRP conjugated compact polymer system. DAB was used as the chromogen. The section was then counterstained with haematoxylin and mounted with DPX. The inset secondary-only control image is taken from an identical assay without primary antibody.

For other IHC staining systems (automated and non-automated) customers should optimize variable parameters such as antigen retrieval conditions, primary antibody concentration and antibody incubation times.


**Tissue obtained from the Human Research Tissue Bank, supported by the NIHR Cambridge Biomedical Research Centre*

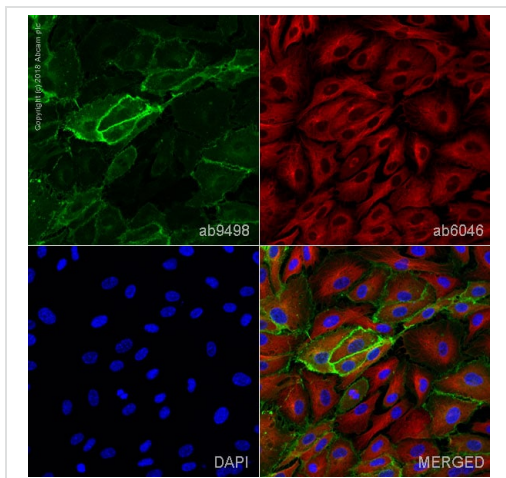

Immunocytochemistry/ Immunofluorescence - Anti-CD31 antibody [JC/70A] (ab9498)

ab9498 staining CD31 in HUVEC cells. The cells were fixed with 4% formaldehyde (10min), permeabilized with 0.1%PBS-Tween for 5 minutes and then blocked with 1% BSA/10% normal goat serum/0.3M glycine in 0.1%PBS-Tween for 1h. The cells were then incubated overnight at +4°C with ab9498 at 1µg/ml and **ab6046**, Rabbit polyclonal to beta Tubulin - Loading Control, at 1/1000 dilution. Cells were then incubated with **ab150117**, Goat Anti-Mouse IgG H&L (Alexa Fluor® 488) at 1/1000 dilution (shown in green) and **ab150084**, Goat polyclonal Secondary Antibody to Rabbit IgG - H&L (Alexa Fluor® 594) at 1/1000 dilution (shown in pseudocolor red). Nuclear DNA was labelled with DAPI (shown in blue).

Image was taken with a confocal microscope (Leica-Microsystems, TCS SP8).

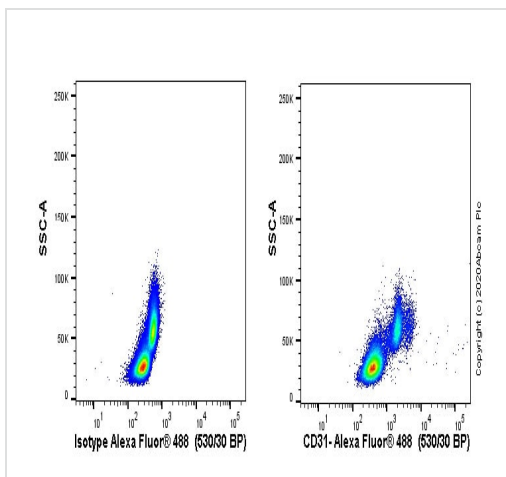


Flow Cytometry - Anti-CD31 antibody [JC/70A] (ab9498)

Flow cytometry staining of human peripheral blood mononuclear cells (PBMCs) with ab9498 (right) or mouse IgG1κ; (**ab170190**) isotype (left). PBMCs were incubated for 30 min on ice in 1x PBS containing 10 µg/ml human IgG and 10% normal goat serum to block FC receptors and non-specific protein-protein interaction followed by the antibody (ab9498) or mouse IgG1κ; (**ab170190**) isotype (1x10⁶ in 100 µL at 0.04 µg/ml) for 30 min on ice.

The secondary antibody Goat anti-mouse IgG H&L (Alexa Fluor® 488, pre-adsorbed) (**ab150117**) was used at 1:2000 dilution for 30 min on ice.

Acquisition of >30000 events were collected using a 50 mW Blue laser (488nm) and 530/30 bandpass filter. Events were gated on alive cells.

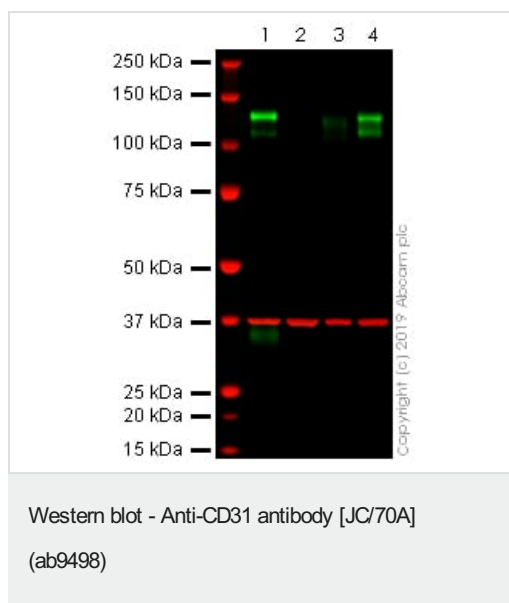

All lanes : Anti-CD31 antibody [JC/70A] (ab9498) at 1 µg/ml

Lane 1 : HUVEC whole cell lysate

Lane 2 : HeLa whole cell lysate

Lane 3 : Human kidney tissue lysate

Lane 4 : Human spleen tissue lysate


Lysates/proteins at 20 µg per lane.

Performed under reducing conditions.

Predicted band size: 82 kDa

Observed band size: 130 kDa

This blot was produced using a 4-12% Bis-tris under the MOPS buffer system. The gel was run at 200V for 55 minutes before being transferred onto a Nitrocellulose membrane at 30V for 70 minutes. The membrane was blocked for an hour using 3% milk before ab9498 and [ab181602](#) (Rabbit anti-GAPDH loading control) were incubated overnight at 4°C at a 1ug/ml concentration and 1/20000 dilution respectively. Antibody binding was detected using Goat anti-Mouse IgG H&L (IRDye® 800CW) preadsorbed ([ab216772](#)) and Goat anti-Rabbit IgG H&L (IRDye® 680RD) preadsorbed ([ab216777](#)) secondary antibodies at 1/20000 dilution for 1 hour at room temperature before imaging.

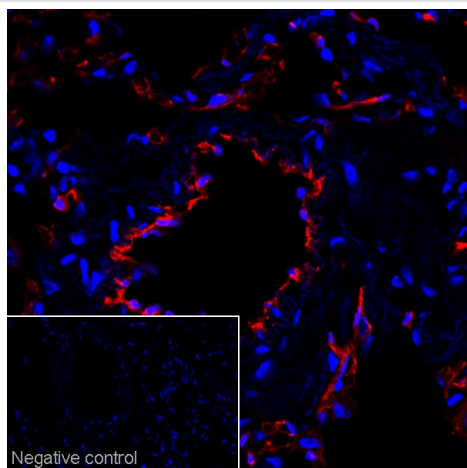


Immunohistochemistry (Frozen sections) - Anti-CD31 antibody [JC/70A] (ab9498)

IHC image of ab9498 staining in 10% formaldehyde fixed frozen tissue section of human lung.

Non-specific protein-protein interactions were blocked using TBS containing 0.025% (v/v) Triton X-100, 0.3M (w/v) glycine and 3% (w/v) BSA for 1 hour at room temperature. The section was then incubated with ab9498 (1 µg/ml concentration) in TBS containing 0.025% (v/v) Triton X-100 and 3% (w/v) BSA overnight at +4°C. The section was then incubated with **ab150119** (Goat polyclonal Secondary Antibody to Mouse IgG - H&L (Alexa Fluor® 647)) and DAPI for 1 hour at room temperature.

The DAPI only control (no antibody) inset shows no autofluorescence, demonstrating that any Alexa Fluor® 647 signal is derived directly from bound ab9498.

For other IHC staining systems (automated and non-automated), customers should optimize variable parameters such as antibody concentrations and incubation times.

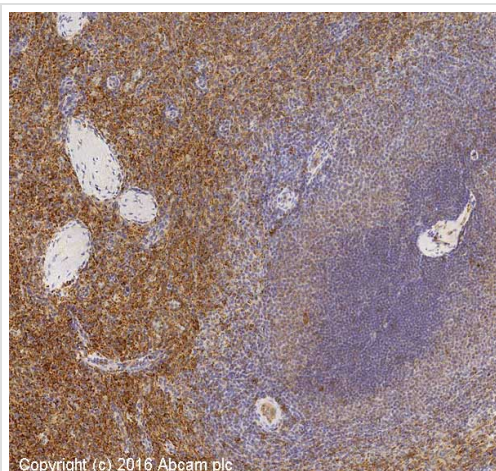


Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-CD31 antibody [JC/70A] (ab9498)

IHC image of CD31 staining in human spleen formalin fixed paraffin embedded tissue section*, performed on a Leica Bond™ system using the standard protocol F. The section was pre-treated using heat mediated antigen retrieval with sodium citrate buffer (pH6, epitope retrieval solution 1) for 20 mins. The section was then incubated with ab9498, 5 µg/ml, for 15 mins at room temperature and detected using an HRP conjugated compact polymer system. DAB was used as the chromogen. The section was then counterstained with haematoxylin and mounted with DPX.

For other IHC staining systems (automated and non-automated) customers should optimize variable parameters such as antigen retrieval conditions, primary antibody concentration and antibody incubation times.


**Tissue obtained from the Human Research Tissue Bank, supported by the NIHR Cambridge Biomedical Research Centre*

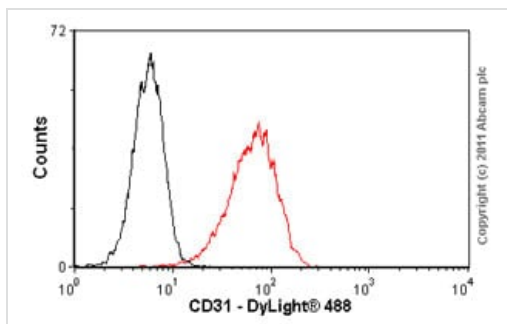

Flow Cytometry - Anti-CD31 antibody [JC/70A]
(ab9498)


Overlay histogram showing Jurkat cells stained with ab9498 (red line). The cells were fixed with 4% paraformaldehyde (10 min) and incubated in 1x PBS / 10% normal goat serum / 0.3M glycine to block non-specific protein-protein interactions. The cells were then incubated with the antibody (ab9498, 1/20 dilution) for 30 min at 22°C. The secondary antibody used was DyLight® 488 goat anti-mouse IgG (H+L) ([ab96879](#)) at 1/500 dilution for 30 min at 22°C. Isotype control antibody (black line) was mouse IgG1 [ICIGG1] ([ab91353](#), 2µg/1x10⁶ cells) used under the same conditions. Acquisition of >5,000 events was performed. This antibody gave a positive signal in Jurkat cells fixed with methanol (5 min) used under the same conditions.

Please note that Abcam do not have data for use of this antibody on non-fixed cells. We welcome any customer feedback.

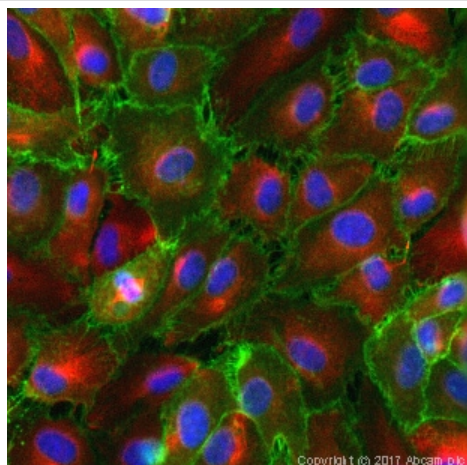


Immunocytochemistry/ Immunofluorescence - Anti-
CD31 antibody [JC/70A] (ab9498)

ab9498 stained in HUVEC cells. Cells were fixed with 100% methanol (5 min) at room temperature and incubated with PBS containing 10% goat serum, 0.3 M glycine, 1% BSA and 0.1% tween for 1h at room temperature to permeabilise the cells and block non-specific protein-protein interactions. The cells were then incubated with the antibody ab9498 at 5 µg/ml and [ab6046](#) (Rabbit polyclonal to beta Tubulin) at 1/1000 dilution overnight at +4°C. The secondary antibodies were [ab150080](#) (pseudo-colored red) and [ab150117](#) (colored green) used at 1 µg/ml for 1 hour at room temperature. DAPI was used to stain the cell nuclei (colored blue) at a concentration of 1.43µM for 1 hour at room temperature

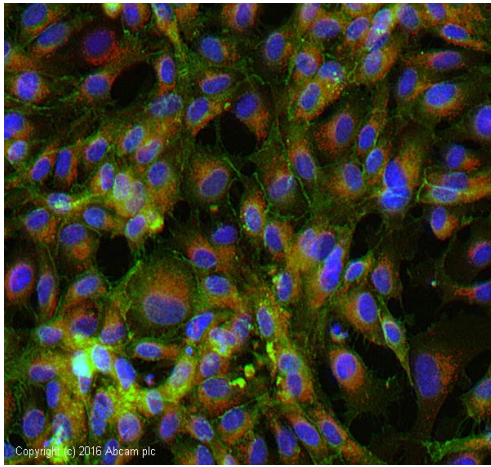

Immunocytochemistry/ Immunofluorescence - Anti-CD31 antibody [JC/70A] (ab9498)

ab9498 stained HUVEC cells. The cells were 100% methanol fixed for 5 minutes at -20°C and then incubated in 1%BSA / 10% normal goat serum / 0.3M glycine in 0.1% PBS-Tween for 1hour at room temperature to permeabilise the cells and block non-specific protein-protein interactions. The cells were then incubated with the antibody (ab9498 at 5µg/ml) overnight at +4°C. The secondary antibody (pseudo-colored green) was **Goat Anti-Mouse IgG H&L (Alexa Fluor® 488) preadsorbed (ab150117)** used at a 1/1000 dilution for 1hour at room temperature. Alexa Fluor® 594 WGA was used to label plasma membranes (pseudo-colored red) at a 1/200 dilution for 1hour at room temperature. DAPI was used to stain the cell nuclei (pseudo-colored blue) at a concentration of 1.43µM for 1hour at room temperature.

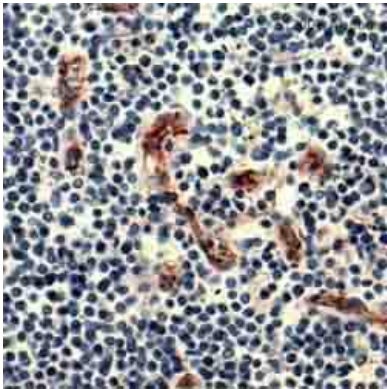

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-CD31 antibody [JC/70A] (ab9498)

This image is courtesy of an anonymous Abreview

ab9498 at 1/100 staining human lymph node tissue sections by IHC-P. The tissue was paraformaldehyde fixed and a heat based antigen retrieval step was performed. The tissue was then blocked with serum and incubated with ab9498 overnight. An HRP conjugated goat antibody was used as the secondary.

Please note: All products are "FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES"

Our Abpromise to you: Quality guaranteed and expert technical support

- Replacement or refund for products not performing as stated on the datasheet
- Valid for 12 months from date of delivery
- Response to your inquiry within 24 hours
- We provide support in Chinese, English, French, German, Japanese and Spanish
- Extensive multi-media technical resources to help you
- We investigate all quality concerns to ensure our products perform to the highest standards

If the product does not perform as described on this datasheet, we will offer a refund or replacement. For full details of the Abpromise, please visit <https://www.abcam.co.jp/abpromise> or contact our technical team.

Terms and conditions

- Guarantee only valid for products bought direct from Abcam or one of our authorized distributors