

# Anti-HLA Class I antibody [W6/32] - BSA and Azide free ab23755

リコンビナント

★★★★★ **5 Abreviews**   **16 References**   画像数 4

### 製品の概要

製品名	Anti-HLA Class I antibody [W6/32] - BSA and Azide free
製品の詳細	Mouse monoclonal [W6/32] to HLA Class I - BSA and Azide free
由来種	Mouse
アプリケーション	<b>適用あり:</b> Flow Cyt, ICC/IF, IHC-Fr
種交差性	<b>交差種:</b> Human
免疫原	Tissue, cells or virus corresponding to Human HLA Class I. Membrane of human tonsil cells
ポジティブ・コントロール	IHC-Fr: Human heart tissue. ICC/IF: HeLa cells. Flow Cyt: Jurkat cells.
特記事項	<p>This product has switched from a hybridoma to recombinant production method on 25th March 2024.</p> <p>This product is a recombinant monoclonal antibody, which offers several advantages including:</p> <ul style="list-style-type: none"> <li>- High batch-to-batch consistency and reproducibility</li> <li>- Improved sensitivity and specificity</li> <li>- Long-term security of supply</li> <li>- Animal-free production</li> </ul> <p>For more information <a href="#">see here</a>.</p>

### 製品の特性

製品の状態	Liquid
保存方法	Shipped at 4°C. Store at +4°C. Do Not Freeze.
バッファー	pH: 7.2 Constituent: 100% PBS
キャリア・フリー	はい
精製度	Protein A purified
一次抗体 備考	The antibody recognises virtually all nucleated human cells, it is a valuable reagent for analysing variations in HLA class I expression in different disease states e.g. liver disease, muscular dystrophy, inflammatory myopathy and other neuromuscular disorders. This antibody is also suitable as a positive control for HLA tissue typing and crossmatching.

ポリ/モノ	モノクローナル
クローン名	W6/32
アイソタイプ	IgG2a

## アプリケーション

The Abpromise guarantee      **Abpromise保証は、** 次のテスト済みアプリケーションにおけるab23755の使用に適用されます  
 アプリケーションノートには、推奨の開始希釈率がありますが、適切な希釈率につきましてはご検討ください。


アプリケーション	Abreviews	特記事項
Flow Cyt	★★★★★ (2)	Use at an assay dependent concentration.
ICC/IF		Use at an assay dependent concentration.
IHC-Fr		Use at an assay dependent concentration.

## ターゲット情報


関連性	HLA CClass I is involved in the presentation of foreign antigens to the immune system.
細胞内局在	Plasma membrane

## 画像

Frozen Human Spleen




Frozen Human Heart

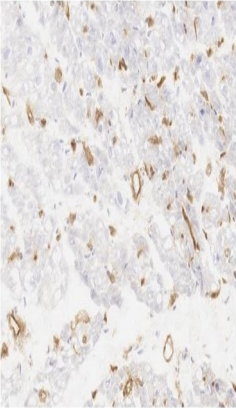

Immunohistochemistry (Frozen sections) - Anti-HLA Class I antibody [W6/32] - BSA and Azide free (ab23755)

This data was developed using **ab22432**, the same antibody clone in a different buffer formulation.


Immunohistochemical analysis of **ab22432** 10% paraformaldehyde fixed endothelial cells in frozen Human spleen tissue Human heart tissue labeling HLA Class I with **ab22432** at 0.05µg/ml. Detected using an HRP conjugated compact polymer system. DAB was used as the chromogen. The section was then counterstained with haematoxylin and mounted with DPX.

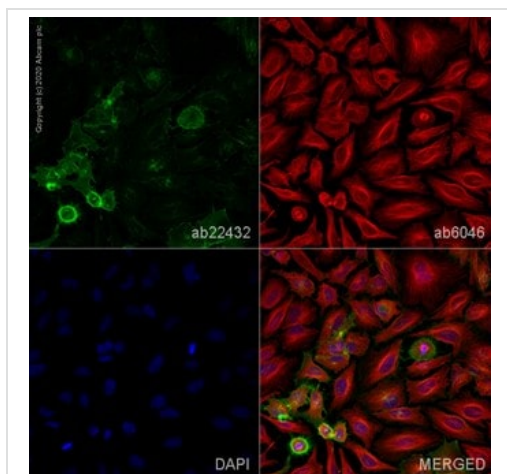

Immunocytochemistry/ Immunofluorescence - Anti-HLA Class I antibody [W6/32] - BSA and Azide free (ab23755)

This data was developed using [ab22432](#), the same antibody clone in a different buffer formulation.


Immunofluorescent analysis of 4% Paraformaldehyde-fixed, 0.1% PBS-Tween permeabilized HeLa (human cervical adenocarcinoma epithelial cell) cells labelling HLA Class I with [ab22432](#) at 1µg/mL, blocked with 1% BSA/10% normal goat serum/0.3M glycine in 0.1%PBS-Tween for 1h. The cells were then incubated overnight at 4°C with [ab92494](#) at 1µg/mL and [ab6046](#), Rabbit polyclonal to beta Tubulin - Loading Control. Cells were then incubated with [ab150117](#), Goat polyclonal Secondary Antibody to Mouse IgG H&L (Alexa Fluor® 488) preadsorbed at 1/1000 dilution (shown in green) and [ab150080](#), Goat polyclonal Secondary Antibody to Rabbit IgG - H&L (Alexa Fluor® 594) at 1/1000 dilution (shown in red). Nuclear DNA was labelled with DAPI (shown in blue). Image was acquired with a high-content analyser (Operetta CLS, Perkin Elmer) and a maximum intensity projection of confocal sections is shown.

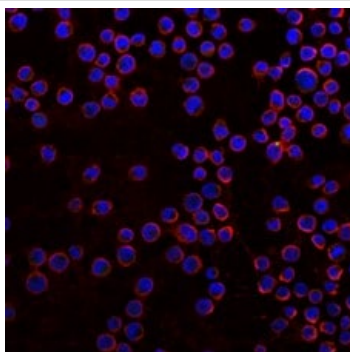

Immunocytochemistry/ Immunofluorescence - Anti-HLA Class I antibody [W6/32] - BSA and Azide free (ab23755)

This data was developed using [ab22432](#), the same antibody clone in a different buffer formulation.

Immunofluorescent analysis of 4% Paraformaldehyde-fixed, 0.1% PBS-Tween permeabilized negative cell line K562 labelling HLA Class I with [ab22432](#) at 1µg/mL, blocked with 1% BSA/10% normal goat serum/0.3M glycine in 0.1%PBS-Tween for 1h. The cells were then incubated overnight at 4°C with [ab227805](#) at 5µg/ml and [ab6046](#), Rabbit polyclonal to beta Tubulin - Loading Control. Cells were then incubated with [ab150117](#), Goat polyclonal Secondary Antibody to Mouse IgG H&L (Alexa Fluor® 488) preadsorbed at 1/1000 dilution (shown in green) and [ab150080](#), Goat polyclonal Secondary Antibody to Rabbit IgG - H&L (Alexa Fluor® 594) at 1/1000 dilution (shown in red). Nuclear DNA was labelled with DAPI (shown in blue). Also suitable in cells fixed with 100% methanol (5 min). Image was acquired with a confocal microscope (Leica-Microsystems TCS SP8) and a single confocal section is shown.

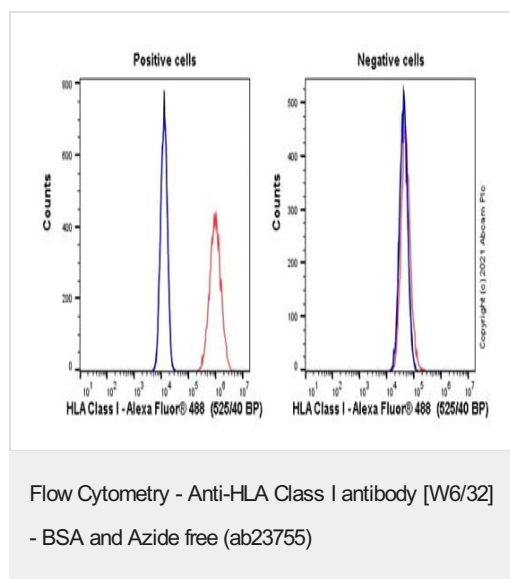

This data was developed using **ab22432**, the same antibody clone in a different buffer formulation.

Flow cytometry overlay histogram showing left Jurkat positive cells and right negative K562 cells stained with **ab22432** (red line). The cells were incubated in 1x PBS containing 10 % normal goat serum to block non-specific protein-protein interaction followed by the antibody (**ab22432**) ( $1 \times 10^6$  in 100  $\mu$ l at 0.2  $\mu$ g/ml) for 30 min on ice. The secondary antibody Goat anti-mouse IgG H&L (Alexa Fluor® 488, pre-adsorbed) (**ab150117**) was used at for 30 min on ice. Isotype control antibody (black line) was mouse IgG2a (**ab18413**) used at the same concentration and conditions as the primary antibody. Unlabeled sample (blue line) was also used as a control. Acquisition of >5000 events were collected using a 50 mW Blue laser (488nm) and 525/40 bandpass filter.

**Please note:** All products are "FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES"

## Our Abpromise to you: Quality guaranteed and expert technical support

- Replacement or refund for products not performing as stated on the datasheet
- Valid for 12 months from date of delivery
- Response to your inquiry within 24 hours
- We provide support in Chinese, English, French, German, Japanese and Spanish
- Extensive multi-media technical resources to help you
- We investigate all quality concerns to ensure our products perform to the highest standards

If the product does not perform as described on this datasheet, we will offer a refund or replacement. For full details of the Abpromise, please visit <https://www.abcam.co.jp/abpromise> or contact our technical team.

## Terms and conditions

- Guarantee only valid for products bought direct from Abcam or one of our authorized distributors