

Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] ab254222

KO 評価済 リコンビナント RabMAb

★★★★★ [1 Abreviews](#) [12 References](#) [画像数 14](#)

製品の概要

製品名	Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247]
製品の詳細	Rabbit monoclonal [EPR22291-247] to Angiotensin Converting Enzyme 1
由来種	Rabbit
アプリケーション	適用あり: IHC-Fr, WB, IHC-P, mIHC, Indirect ELISA 適用なし: Flow Cyt, ICC/IF or IP
種交差性	交差種: Mouse, Rat, Human
免疫原	Recombinant fragment. This information is proprietary to Abcam and/or its suppliers.
ポジティブ・コントロール	WB: bEND.3, HUVEC and HAP1 whole cell lysates; human kidney and lung cell lysates; mouse brain, heart, kidney, spleen and lung tissue lysates; rat brain, heart, liver and spleen tissue lysates. IHC-P: Human kidney and liver tissue; mouse kidney tissue; rat kidney tissue. IHC-Fr: Mouse kidney tissue; rat kidney tissue. mIHC-P: Human kidney tissue.
特記事項	This product is a recombinant monoclonal antibody, which offers several advantages including: <ul style="list-style-type: none"> - High batch-to-batch consistency and reproducibility - Improved sensitivity and specificity - Long-term security of supply - Animal-free production For more information see here . Our RabMAb [®] technology is a patented hybridoma-based technology for making rabbit monoclonal antibodies. For details on our patents, please refer to RabMAb[®] patents .

製品の特性

製品の状態	Liquid
保存方法	Shipped at 4°C. Store at +4°C short term (1-2 weeks). Upon delivery aliquot. Store at -20°C long term. Avoid freeze / thaw cycle.
バッファー	pH: 7.2 Preservative: 0.01% Sodium azide Constituents: PBS, 40% Glycerol, 0.05% BSA

精製度	Protein A purified
ポリ/モノ	モノクローナル
クローン名	EPR22291-247
アイソタイプ	IgG

アプリケーション

The Abpromise guarantee **Abpromise保証は、次のテスト済みアプリケーションにおけるab254222の使用に適用されます**
 アプリケーションノートには、推奨の開始希釈率がありますが、適切な希釈率につきましてはご検討ください。

アプリケーション	Abreviews	特記事項
IHC-Fr		1/500. Heat mediated antigen retrieval using sodium citrate buffer (10mM citrate pH 6.0 + 0.05% Tween-20).
WB	★★★★★ (1)	1/1000. Detects a band of approximately 180 kDa (predicted molecular weight: 150 kDa).
IHC-P		1/4000. Perform heat mediated antigen retrieval with Tris/EDTA buffer pH 9.0 before commencing with IHC staining protocol.
mIHC		1/4000.
Indirect ELISA		Use at an assay dependent concentration.

追加情報 Is unsuitable for Flow Cyt, ICC/IF or IP.

ターゲット情報

機能	Converts angiotensin I to angiotensin II by release of the terminal His-Leu, this results in an increase of the vasoconstrictor activity of angiotensin. Also able to inactivate bradykinin, a potent vasodilator. Has also a glycosidase activity which releases GPI-anchored proteins from the membrane by cleaving the mannose linkage in the GPI moiety.
組織特異性	Ubiquitously expressed, with highest levels in lung, kidney, heart, gastrointestinal system and prostate. Isoform Testis-specific is expressed in spermatocytes and adult testis.
関連疾患	<p>Ischemic stroke (ISCHSTR) [MIM:601367]: A stroke is an acute neurologic event leading to death of neural tissue of the brain and resulting in loss of motor, sensory and/or cognitive function. Ischemic strokes, resulting from vascular occlusion, is considered to be a highly complex disease consisting of a group of heterogeneous disorders with multiple genetic and environmental risk factors. Note=Disease susceptibility is associated with variations affecting the gene represented in this entry.</p> <p>Renal tubular dysgenesis (RTD) [MIM:267430]: Autosomal recessive severe disorder of renal tubular development characterized by persistent fetal anuria and perinatal death, probably due to pulmonary hypoplasia from early-onset oligohydramnios (the Potter phenotype). Note=The disease is caused by mutations affecting the gene represented in this entry.</p> <p>Microvascular complications of diabetes 3 (MVCD3) [MIM:612624]: Pathological conditions that develop in numerous tissues and organs as a consequence of diabetes mellitus. They include diabetic retinopathy, diabetic nephropathy leading to end-stage renal disease, and diabetic</p>

neuropathy. Diabetic retinopathy remains the major cause of new-onset blindness among diabetic adults. It is characterized by vascular permeability and increased tissue ischemia and angiogenesis. Note=Disease susceptibility is associated with variations affecting the gene represented in this entry.

Intracerebral hemorrhage (ICH) [MIM:614519]: A pathological condition characterized by bleeding into one or both cerebral hemispheres including the basal ganglia and the cerebral cortex. It is often associated with hypertension and craniocerebral trauma. Intracerebral bleeding is a common cause of stroke. Note=Disease susceptibility is associated with variations affecting the gene represented in this entry.

配列類似性

Belongs to the peptidase M2 family.


翻訳後修飾

Phosphorylated by CK2 on Ser-1299; which allows membrane retention.

細胞内局在

Secreted and Cell membrane.

画像

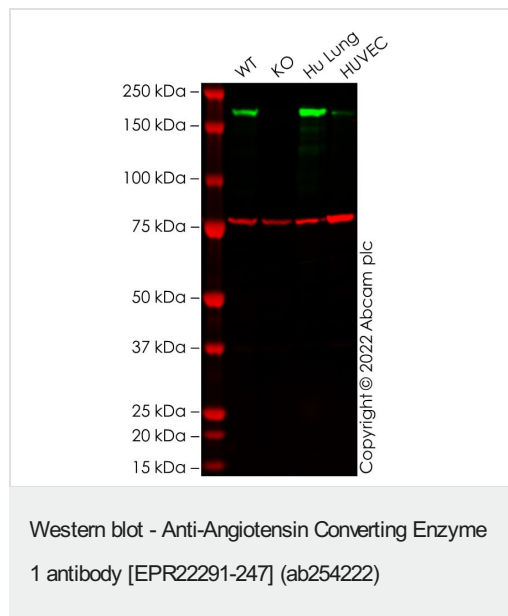

All lanes : Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222) at 1/1000 dilution

Lane 1 : Wild-type SKNFI cell lysate

Lane 2 : Ace knockout SKNFI cell lysate

Lane 3 : Human Lung cell lysate

Lane 4 : HUVEC cell lysate

Lysates/proteins at 20 µg per lane.


Performed under reducing conditions.

Predicted band size: 150 kDa

Observed band size: 200 kDa

False colour image of Western blot: Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] staining at 1/1000 dilution, shown in green; Mouse anti-CANX [CANX/1543] ([ab238078](#)) loading control staining at 1/20000 dilution, shown in red. In Western blot, ab254222 was shown to bind specifically to Angiotensin Converting Enzyme 1. A band was observed at 200 kDa in wild-type SKNFI cell lysates with no signal observed at this size in Ace knockout cell line [ab288707](#). To generate this image, wild-type and Ace knockout SKNFI cell lysates were analysed. First, samples were run on an SDS-PAGE gel then transferred onto a nitrocellulose membrane. Membranes were blocked in 3 % milk in TBS-0.1 % Tween® 20 (TBS-T) before incubation with primary

antibodies overnight at 4 °C. Blots were washed four times in TBS-T, incubated with secondary antibodies for 1 h at room temperature, washed again four times then imaged. Secondary antibodies used were Goat anti-Rabbit IgG H&L 800CW and Goat anti-Mouse IgG H&L 680RD at 1/20000 dilution.

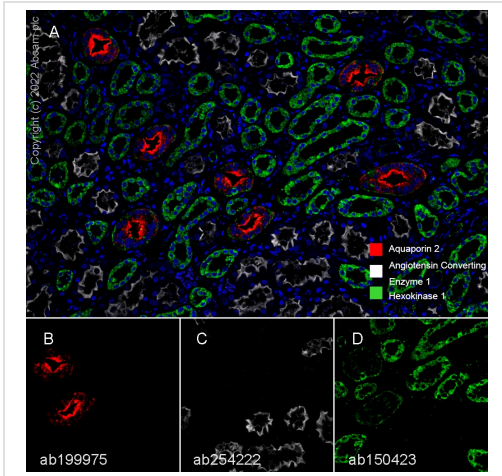

Multiplex immunohistochemistry - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)


Fluorescence multiplex immunohistochemical analysis of the human kidney (Formalin/PFA-fixed paraffin-embedded sections).

Panel A: merged staining of anti-Hexokinase 1 (**ab150423**, green; Opal™690), anti-Angiotensin Converting Enzyme 1 (ab254222, gray; Opal™520) and anti-Aquaporin 2 (**ab199975**, red; Opal™570) on human kidney. Panel B: anti-Aquaporin 2 stained on collecting tubules. Panel C: anti-Angiotensin Converting Enzyme 1 stained on proximal tubules. Panel D: anti-Hexokinase 1 stained on distal tubules and collecting tubules. Opal Polymer HRP Ms + Rb was used as a secondary antibody.

The section was incubated in three rounds of staining: in the order of **ab150423** at 1/250 dilution (4.224 µg/ml), ab254222 at 1/4000 dilution (0.141 µg/ml) and **ab199975** at 1/4000 dilution (0.152 µg/ml) for 30 mins at room temperature. Each round was followed by a separate fluorescent tyramide signal amplification system.

The immunostaining was performed on a Leica Biosystems BOND® RX instrument with an Opal™ 4-color kit. Image acquisition was performed with Leica SP8 confocal microscope.

Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution2) for 20 mins. DAPI (blue) was used as a nuclear counter stain.

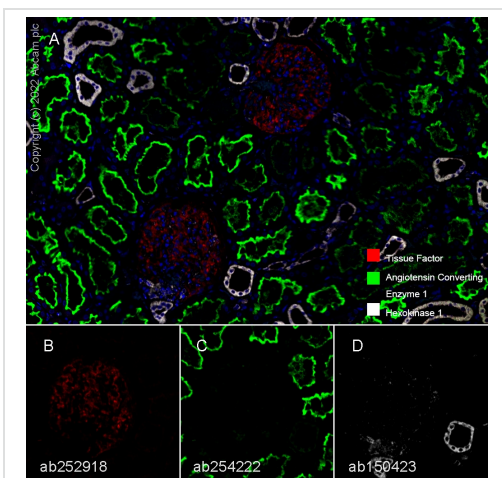

Multiplex immunohistochemistry - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

Fluorescence multiplex immunohistochemical analysis of paraffin-embedded Human kidney tissue.

Panel A: Merged staining of anti-Hexokinase 1 (gray; Opal™690), anti-Angiotensin Converting Enzyme 1 (green; Opal™520) and anti-Tissue Factor (red; Opal™570) on human kidney.


Panel B: Anti-Tissue Factor stained on renal glomeruli.

Panel C: Anti-Angiotensin Converting Enzyme 1 stained on proximal tubules.

Panel D: Anti-Hexokinase 1 stained on distal tubules.

The section was incubated in three rounds of staining: in the order of **ab150423**, ab254222, and **ab252918** for 30 mins at room temperature. Each round was followed by a separate fluorescent tyramide signal amplification system. The immunostaining was performed on a Leica Biosystems BOND® RX instrument with an

Opal™ 4-color kit. Image acquisition was performed with Leica SP8 confocal microscope. Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution 2) for 20 mins. Counterstained with DAPI.

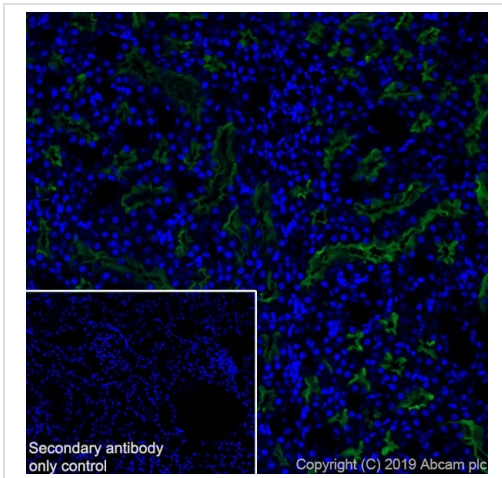


Immunohistochemistry (Frozen sections) - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

Immunohistochemical analysis of frozen section of 4% PFA-fixed, 0.2% Triton X-100 permeabilized rat kidney tissue labeling Angiotensin Converting Enzyme 1 with ab254222 at 1/500 dilution, followed by Goat Anti-Rabbit IgG H&L (Alexa Fluor® 488) (**ab150077**) at 1/1000 dilution (green). Positive staining on proximal tubules of kidney (PMID:10504496) is observed. The nuclear counter stain is DAPI (blue).

Secondary antibody only control: Used PBS instead of primary antibody, secondary antibody is Goat Anti-Rabbit IgG H&L (Alexa Fluor® 488) (**ab150077**) at 1/1000 dilution.

Heat mediated antigen retrieval using sodium citrate buffer (10mM citrate pH 6.0 + 0.05% Tween-20).

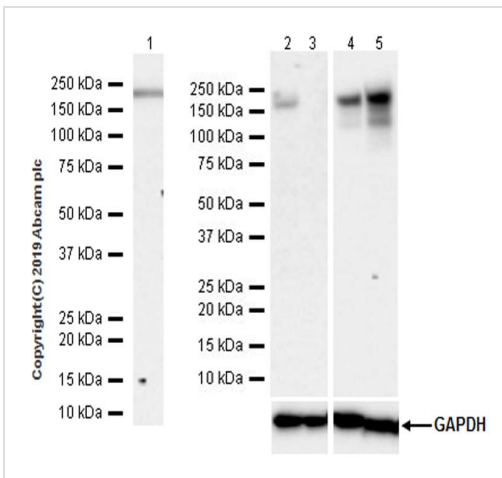

Western blot - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

All lanes : Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222) at 1/1000 dilution

Lane 1 : HUVEC (human umbilical vein endothelial cell line) whole cell lysate at 20 µg

Lane 2 : Wild-type HAP1 whole cell lysate at 40 µg

Lane 3 : Angiotensin Converting Enzyme 1 knockout HAP1 whole cell lysate at 40 µg

Lane 4 : Human kidney cell lysate at 40 µg

Lane 5 : Human lung cell lysate at 40 µg

Secondary

All lanes : Goat Anti-Rabbit IgG H&L (HRP) (**ab97051**) at 1/100000 dilution

Developed using the ECL technique.

Predicted band size: 150 kDa

Observed band size: 180 kDa


Blocking and dilution buffer: 5% NFDm/TBST.

Exposure times.

Lanes 1-3: 3 minutes. Lanes 4-5: 5.5 seconds.

ab254222 was shown to specifically react with Angiotensin Converting Enzyme 1 in wild-type HAP1 cells as signal was lost in Angiotensin Converting Enzyme 1 knockout cells. Wild-type and Angiotensin Converting Enzyme 1 knockout samples were subjected to SDS-PAGE. ab254222 and **ab181602** (Rabbit anti-GAPDH loading control) were incubated 1 hour at room temperature at 1/1000 dilution and 1/200,000 dilution respectively. Blots were developed with Goat Anti-Rabbit IgG, (H+L), Peroxidase conjugated (**ab97051**) secondary antibody at 1/100,000 dilution for 1 hour at room temperature before imaging. The blot was developed on a BIO-RAD[®] ChemiDoc[™] MP instrument using the ECL technique.

The molecular weight observed, and the expression profile are consistent with what have been described in the literature (PMID: 25495544, 16203874).

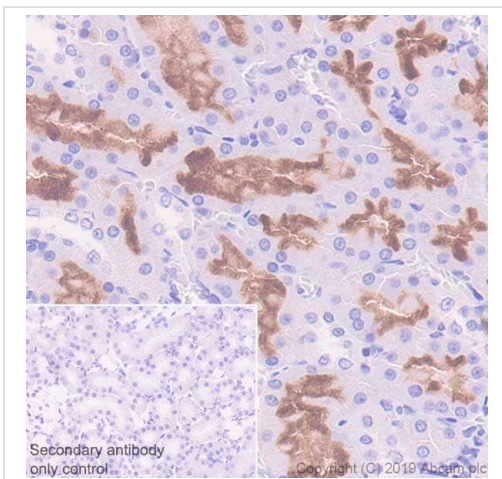

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)


Immunohistochemical analysis of paraffin-embedded rat kidney tissue labeling Angiotensin Converting Enzyme 1 with ab254222 at 1/4000 dilution, followed by a Rabbit specific IHC polymer detection kit HRP/DAB (**ab209101**). Positive staining on proximal tubules of mouse kidney (PMID: 2828286; PMID: 175444) is observed. Counter stained with hematoxylin.

Secondary antibody only control: Used PBS instead of primary antibody, secondary antibody is Rabbit specific IHC polymer detection kit HRP/DAB (**ab209101**).

Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution 2) for 20 mins.

The section was incubated with ab254222 for 30 mins at room temperature.

The immunostaining was performed on a Leica Biosystems BOND[®] RX instrument.

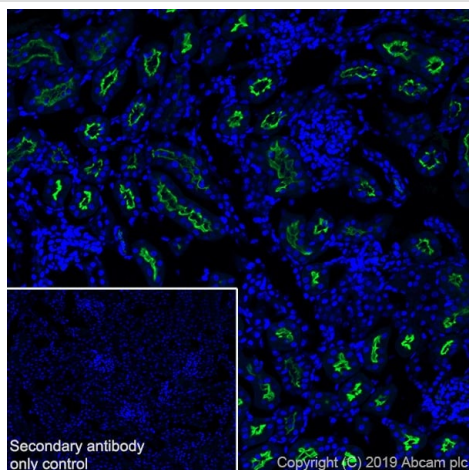


Immunohistochemistry (Frozen sections) - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

Immunohistochemical analysis of frozen section of 4% PFA-fixed, 0.2% Triton X-100 permeabilized mouse kidney tissue labeling Angiotensin Converting Enzyme 1 with ab254222 at 1/500 dilution, followed by Goat Anti-Rabbit IgG H&L (Alexa Fluor® 488) (**ab150077**) at 1/1000 dilution (green). Positive staining on proximal tubules of kidney (PMID:10504496) is observed. The nuclear counter stain is DAPI (blue).

Secondary antibody only control: Used PBS instead of primary antibody, secondary antibody is Goat Anti-Rabbit IgG H&L (Alexa Fluor® 488) (**ab150077**) at 1/1000 dilution.

Heat mediated antigen retrieval using sodium citrate buffer (10mM citrate pH 6.0 + 0.05% Tween-20).

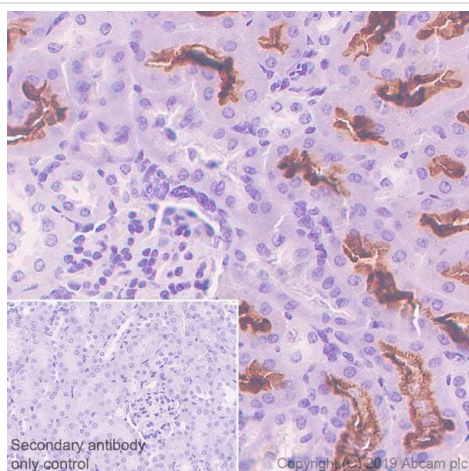

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)


Immunohistochemical analysis of paraffin-embedded mouse kidney tissue labeling Angiotensin Converting Enzyme 1 with ab254222 at 1/4000 dilution, followed by Rabbit specific IHC polymer detection kit HRP/DAB (**ab209101**). Positive staining on proximal tubules in mouse kidney (PMID: 2828286; PMID: 175444) is observed. Counter stained with hematoxylin.

Secondary antibody only control: Used PBS instead of primary antibody, secondary antibody is Rabbit specific IHC polymer detection kit HRP/DAB (**ab209101**).

Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution 2) for 20 mins.

The section was incubated with ab254222 for 30 mins at room temperature.

The immunostaining was performed on a Leica Biosystems BOND® RX instrument.

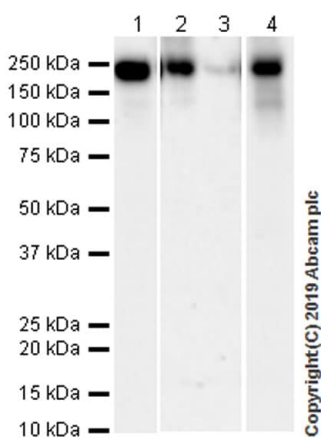

Western blot - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

All lanes : Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222) at 1/1000 dilution

Lane 1 : Rat brain tissue lysate

Lane 2 : Rat heart tissue lysate

Lane 3 : Rat liver tissue lysate

Lane 4 : Rat spleen tissue lysate

Lysates/proteins at 20 µg per lane.

Secondary

All lanes : Goat Anti-Rabbit IgG H&L (HRP) ([ab97051](#)) at 1/100000 dilution


Predicted band size: 150 kDa

Observed band size: 180 kDa

Blocking and dilution buffer: 5% NFDm/TBST.

Exposure times.

Lane 1: 48 seconds. Lanes 2 & 3: 3 minutes. Lane 4: 48 seconds.

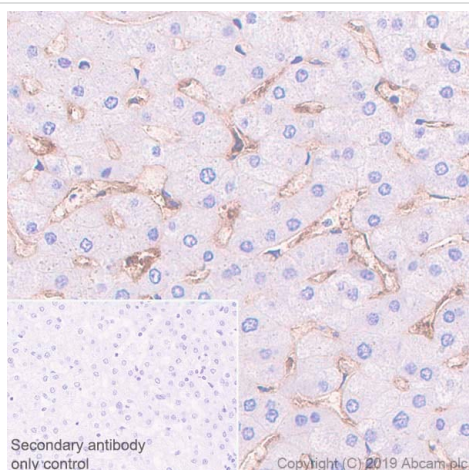

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)


Immunohistochemical analysis of paraffin-embedded human liver tissue labeling Angiotensin Converting Enzyme 1 with ab254222 at 1/4000 dilution, followed by Rabbit specific IHC polymer detection kit HRP/DAB ([ab209101](#)). Positive staining on blood vessels of human liver (PMID: 175444) is observed. Counter stained with hematoxylin.

Secondary antibody only control: Used PBS instead of primary antibody, secondary antibody is Rabbit specific IHC polymer detection kit HRP/DAB ([ab209101](#)).

Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution 2) for 20 mins.

The section was incubated with ab254222 for 30 mins at room temperature.

The immunostaining was performed on a Leica Biosystems BOND® RX instrument.

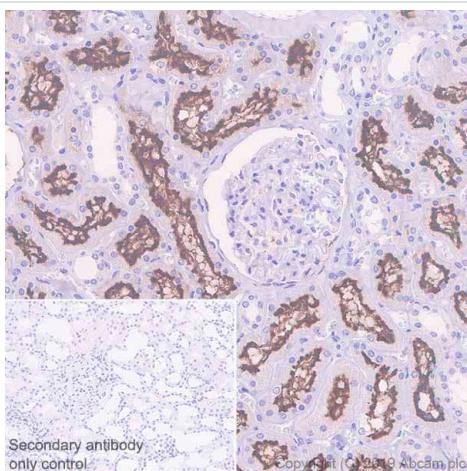

Immunohistochemistry (Formalin/PFA-fixed paraffin-embedded sections) - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)


Immunohistochemical analysis of paraffin-embedded human kidney tissue labeling Angiotensin Converting Enzyme 1 with ab254222 at 1/4000 dilution, followed by Rabbit specific IHC polymer detection kit HRP/DAB (**ab209101**). Positive staining on proximal tubules of human kidney (PMID: 2828286; PMID: 175444) is observed. Counter stained with hematoxylin.

Secondary antibody only control: Used PBS instead of primary antibody, secondary antibody is Rabbit specific IHC polymer detection kit HRP/DAB (**ab209101**).

Heat mediated antigen retrieval with Tris-EDTA buffer (pH 9.0, epitope retrieval solution 2) for 20 mins.

The section was incubated with ab254222 for 30 mins at room temperature.

The immunostaining was performed on a Leica Biosystems BOND[®] RX instrument.

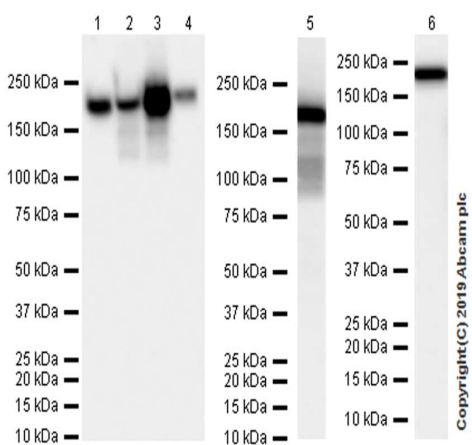

Western blot - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

All lanes : Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222) at 1/1000 dilution

Lane 1 : Mouse brain tissue lysate

Lane 2 : Mouse heart tissue lysate

Lane 3 : Mouse kidney tissue lysate

Lane 4 : Mouse spleen tissue lysate

Lane 5 : Mouse lung tissue lysate

Lane 6 : bEND.3 (mouse brain endothelioma cell line) whole cell lysate

Lysates/proteins at 20 µg per lane.

Secondary

All lanes : Goat Anti-Rabbit IgG H&L (HRP) (**ab97051**) at 1/100000 dilution

Predicted band size: 150 kDa


Observed band size: 180 kDa

Blocking and dilution buffer: 5% NFD/MTBST.

Exposure times.

Lanes 1-4: 10 seconds. Lane 5: 5.5 seconds. Lane 6: 48 seconds.


Indirect ELISA antibody dose-response curve antigen at 1000 ng/ml

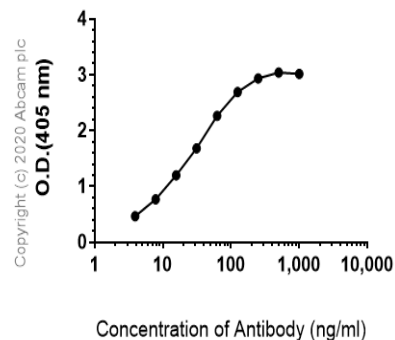

Indirect ELISA - Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

ELISA analysis of ACE recombinant protein at 1000 ng/mL with ab254222. An Alkaline Phosphatase-conjugated AffiniPure Goat Anti-Rabbit IgG (H+L) at 1/2500 dilution was used as the secondary antibody.

Why choose a recombinant antibody?

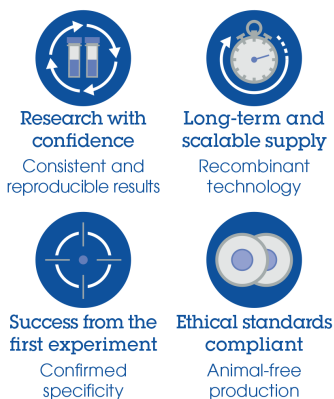

Anti-Angiotensin Converting Enzyme 1 antibody [EPR22291-247] (ab254222)

Please note: All products are "FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES"

Our Abpromise to you: Quality guaranteed and expert technical support

- Replacement or refund for products not performing as stated on the datasheet
- Valid for 12 months from date of delivery
- Response to your inquiry within 24 hours
- We provide support in Chinese, English, French, German, Japanese and Spanish
- Extensive multi-media technical resources to help you
- We investigate all quality concerns to ensure our products perform to the highest standards

If the product does not perform as described on this datasheet, we will offer a refund or replacement. For full details of the Abpromise, please visit <https://www.abcam.co.jp/abpromise> or contact our technical team.

Terms and conditions

- Guarantee only valid for products bought direct from Abcam or one of our authorized distributors